


IONTEST®
Water Simple Analysis kit



NEW DO SENSOR
OXNIT®
OX-V2



NEW DO PROBE
OXNIT®
OSP-2VN

Item	Product Name	Model	Page
1	Water simple Analysis Kit	IONTEST	1
2	MLSS/Sludge Level Meter	SS-10Z	3
3	MLSS Meter	SS-10F	3
4	DO Meter(Dissolved Oxygen Meter)	DO-10Z	4
5	pH/ORP Meter	KP-10Z	4
6	pH Meter	KP-10F	4
7	DO Sensor.....	DO-30N	5
8	MLSS Sensor.....	ML-30N	5
9	2ch DO/pH Meter	DOP-10Z	5
10	Fluoride Ion Meter	F-10Z	6
11	Chloride Ion Meter	CL-10Z	6
12	Chloride Ion Meter	CLCU-55	6
13	Water Quality Testing Unit	10Z Set	7
14	Piston Type,Water Collector	MIZUTEPPPO No.1	7
15	Piston Type,Water Collector	MIZUTEPPPO No.2	7
16	Transparency Tester	AT1~3	8
17	Transparency Tester	JT2~3	8
18	SV Tester(Sludge Deposit rate Tester)	SV-1000	8
19	Dropper Type Water Collector ...	0.5~2m	8
20	Sludge Level Detector	ODEI-pro No.2/No.3	8
21	Scum Thickness Detector	Scummer Z	8
22	Turbidity/Colority Sensor	TCR-5Z	9
23	Turbidity/Colority Sensor	TCR-30	9
24	Turbidity Sensor	TR-30	9
25	Colority Sensor	CR-30	9
26	90° Scattered Light Turbidity Meter	TR-5Z	10
27	SS/Turbidity Sensor	SSTR-5Z	10

Item	Product Name	Model	Page
28	Turbidity Meter	TR-55	10
29	Residual Chlorine Meter(DPD Method)	DP-3F	11
30	High Density Chlorine Meter	RC-3F	11
31	Multi-range Chlorine Meter	RC-V2	11
32	Dissolved Ozone Meter	O ₃ -3F	12
33	Transparency Meter	TP-10Z	12
34	Transparency Meter	TP-30	12
35	Chlorophyll Sensor	CHL-30	13
36	Chlorophyll Sensor	CHL-5Z	13
37	Electric Conductivity Meter	EC-5Z	13
38	Liquid Density Meter	LQ-5Z	14
39	Copper Ion Meter	Cu-V2	14
40	Nickel Ion Meter	Ni-V2	15
41	Hydrogen Peroxide Density Meter	H ₂ O ₂ -V Series	15
42	Sulfuric Acid Meter	H ₂ SO ₄ -55	15
43	Copper Meter	CU-5Z	16
44	Nickel Meter	Ni-5Z/Ni-5ZL	16
45	Copper/Nickel Meter	CuNi-5Z	16
46	Colorimetric Aqua Tester	1Z/2Z Series	17
47	Colorimetric Aqua Tester	7Z Series	17
48	DPD Reagent.....	DPD-F-1/TL-1	17
49	Field Type Water Quality Meters	700/800 Series	18
50	Panel Type Water Quality Meters	502/301 Series	18
51	UV/COD Monitor	UV-700W	19
52	SS/Turbidity Monitor.....	TSS-700W	19
53	Turbidity/Colority Monitor	TCR-700W	19
54	Turbidity Monitor of Laser scattered Light Method	TR-502L	20
55	DO Monitor	DC-502G	20

(※Item 49~55 are relative to Portlab Products)

1 IONTEST® Water Simple Analysis Kit

Anyone can Easily Analyze Water Quality, Anytime and Anywhere.



Exp.:Analysis of Zinc



- ◆ Powder Reagent is sealed up for long/safe validity
- ◆ Convenient for on-site Testing
- ◆ Refined Colorimetry, Ion-Test

Fine transparent Test Cell & 7 colors gradation

Model	Testing item	Range (mg/ℓ = ppm)	Determination Time	Quantity
WIT-Cu	Copper	0.2/0.5/1.0/2.0/3.0/5.0/10 Bicinchoninic Acid method	2min.	50
-Cu(B)	Copper	0.2/0.5/1.0/2.0/3.0/5.0/10 Bathocuproine method ★ If Test water contains such Chelating agent as EDTA, etc., please apply WIT-Cu(B) for testing.	1min.	50
-Ni	Nickel	0.2/0.5/1.0/2.0/3.0/5.0/10 Nioxime method	2min.	50
-NH ₄	Ammonium ion Ammonium-Nitrogen	0.3/0.7/1.3/2.6/6.5/13/26 NH ₄ ⁺ 0.2/0.5/1.0/2.0/5.0/10/20 NH ₄ ⁺ -N Indophenol Blue method	5min.	50
-COD-M	COD-M(Middle range)	0/5/10/13/20/50/100 Oxidation with Potassium Permanganate in Alkalinity method	4~6min.	50
-COD-H	COD-H(High range)	0/20/40/80/120/180/250 Oxidation with Potassium Permanganate in Alkalinity method	4~6min.	50
-Cr ⁶⁺	Chromium(Hexavalent)	0.05/0.1/0.2/0.5/0.8/1.0/2.0 Cr ⁶⁺ Diphenylcarbazide method	2min.	50
-Cr ^T	Total Chromium	0.5/1/2/5/8/10/20 Cr ^T Oxidation and Diphenylcarbazide method	30sec.	50
-HOCl	Residual Chlorine	10/20/30/50/80/100/150 KI method	10sec.	50
-O ₃	Ozone	0.1/0.2/0.3/0.5/0.8/1.0/2.0 DPD method	10sec.	50
-CN	Free Cyanide	0.02/0.05/0.1/0.2/0.5/1.0/2.0 4-Pyridinecarboxylic Acid method	10min.	50
-H ₂ O ₂ -H	Hydrogen Peroxide (High range)	10/20/30/50/80/100/150 KI method	10sec.	50
-NO ₂	Nitrite Nitrite-Nitrogen	0.05/0.1/0.2/0.4/0.6/0.8/1.0 NO ₂ ⁻ 0.015/0.03/0.06/0.12/0.18/0.24/0.30 NO ₂ ⁻ -N GR method	3min.	50
-NO ₃	Nitrate Nitrate-Nitrogen	0.5/1.0/2.0/4.0/6.0/10/20 NO ₃ ⁻ 0.1/0.2/0.5/1.0/1.4/2.3/4.6 NO ₃ ⁻ -N Reduction GR method	3min.	50
-PO ₄	Phosphate Phosphate-Phosphorus	0.2/0.5/1.0/1.5/2.0/3.0/5.0 PO ₄ ³⁻ 0.1/0.2/0.3/0.5/0.7/1.0/1.7 PO ₄ ³⁻ -P Molybdenum blue method	3min.	50
-PO ₄ -H	Phosphate Phosphate-Phosphorus (High range)	2/5/10/15/20/30/50 PO ₄ ³⁻ 0.7/1.7/3.3/5.0/6.6/10/17 PO ₄ ³⁻ -P Molybdenum blue method	3min.	50
-TN-i	Total Nitrogen (Inorganic)	0/5/10/20/40/60/100 Reduction & Indophenol blue method	20min.	50
-Fe	Iron	0.2/0.5/1.0/1.5/2.0/3.0/5.0 Reduction & O-phenanthroline method	5min.	50
-Zn	Zinc	0/0.2/0.3/0.5/1.0/2.0/5.0 PAN method	2min.	50

Where and Which Parameter is IONTEST applied?

for Environmental Research

COD, NO₂, NO₃,
NH₄, PO₄, TN-i, etc.



for Drinking Water Inspection

O₃, HOCl₂, COD, NO₂, NO₃, NH₄,
TN-i, Fe, etc.



for Plating Analysis

Copper, Nickel, Sulfate plating
solution industry.
Cu, Ni, Cr⁶⁺, CN⁻,
PO₄, Fe, Zn,
H₂O₂, etc.



for Waste Water Analysis

Food Factory, Chemical
Factory, Drainage, etc.
COD, TN-i, PO₄, NO₂,
NO₃, NH₄, HOCl₂,
O₃, Cr⁶⁺, Cr⁷⁺, CN⁻,
Zn, etc.



for Fishery Management

COD, NH₄, NO₂, NO₃,
PO₄, TN-i, etc.



for Educational Aid

COD, NO₂, NO₃, NH₄,
TN-i, Cu, Ni, Cr⁶⁺,
HOCl₂, O₃, CN⁻,
H₂O₂, Fe, Zn, etc.



ION TEST Analysis Procedure

1 Add Reagent



Drop reagent into the cell

2 Add Sample



Drop 5 ml or 2ml of sample
into the cell

3 Shake



Shake slightly test cell with lid

4 Colorimetry



Compare to analyze with
standard color card

ION TEST KIT SPECIFICATION



Standard Component

1	Standard Color	1
2	Reagent	50 Pcs.
3	Test Cell	1Pc.
4	Box	1Pc.
5	Pipette	1Pc.




STD Component part is optionally available.


Standard Color (selective)	Reagent (50 pcs) (selective)	Test Cell with Lid (5ml)
WIT-□□□□-STD (EXP. WIT-Cu-STD.)	WIT-□□□□ (EXP. WIT-Cu)	CELL-5C

2 SS-10Z

MLSS / Sludge Level Meter



Sludge level /density measurement in the deposit tank




Measurement of activated sludge density

3 SS-10F

MLSS Meter



(Economy Type)



Measurement of activated sludge density

Features

1 Optional measuring mode (common to SS-10Z and SS-10F)

MODE 1 Food and dairy sludge **A**

MODE 4 Sewage/combine septic tank **B**

MODE 2 Food and dairy sludge **B**

MODE 5 Human waste disposal/deposit tank **A**

MODE 3 Sewage/ combine septic tank **A**

MODE 6 Human waste disposal/deposit tank **B**

2 Simultaneous measurement of MLSS and sludge level (water depth). (SS-10Z)

3 Measured value can be memorized and called back (common)

	SS-10Z (with depth display)	SS-10F (without depth display)
Measuring range	MLSS : 0~20000mg/ℓ (MAX display 30000mg/ℓ)	
	Water depth 0.00~5.00m (max 10m)	none
Accuracy	MLSS: within ± 3% Water depth: within ±0.05m	MLSS: within ± 3%
Detector	SSD-10Z(with pressure sensor)	SSD-10F(without pressure sensor)
Cable length	6m standard(max.11m)	
Carrying case	Standard attachment	

Wide range usage

Septic tank, sewage, MLSS measurement at human waste treatment plant, sludge zone surface of deposit tank, construction site, food, various sludge density of chemical plant.

4 DO-10 Z Dissolved Oxygen Meter (DO Meter)



New DO sensor
OXNIT® OX-V2



New type DO probe **OX-P-2VN**
With strong shock-proofed
rubber protector

2 pin-connector &
double O-ring type

Measuring method	Cartridge type galvanic sensor
Measuring range	DO : 0.00~30.00mg/ℓ
	O ₂ : 0.0~30.0%
	Water temperature : 0.0~50.0℃
DO sensor	OXNIT OX-V2 2 pin type
DO probe	OX-P-2VN (with shock-absorbing rubber protector)

5 KP-10 Z

pH / ORP Meter



6 KP-10 F

pH Meter



Product name	pH / ORP Meter	pH Meter
Model	KP-10Z	KP-10F
Measuring range	0.00~14.00pH	
	0~±1900mV(pH electrode potential)	
	0~±1900mV(ORP)	
	0.0~50.0℃	
Electrode	Collect water type:CE-106	Collect water type:CE-2106
	Throw-in type:CE-120-3	Throw-in type:CE-2120

7 DO-30N DO Sensor(Dissolved Oxygen Meter)

Collecting water type



NEW DO sensor
OXNIT®:OX-V2

2pin-contactor & double O-ring type



Model	DO-30N (Galvanic method)
Display	3 digits LCD display
Measuring range	Dissolved oxygen(DO):0.0~20.0mg/ℓ
	Oxygen in air(O ₂):0.0~30.0%
	Water temperature(TEMP):0.0~50.0℃

8 ML-30N MLSS Sensor(Sludge density meter)

Measurement by collecting water!
0~19900mg/ℓ



Specifications of MLSS detector

Measuring theory

Near-infrared pulse transmitted light method

Product name	Built-in-sensor type MLSS Meter
Model	ML-30N
Display	3·1/2digits LCD
Measuring range	MLSS:0~19900mg/ℓ
Measuring mode	1 point (standard working curve by KRK) ※ Possible to change to user's sample (sludge) in advance.

Water quality inspection flow of aeration tank, drain, etc.



9 DOP-10Z 2ch DO/pH Meter

DO, pH, ORP and water temperature measurement with One Single Unit



New DO sensor
OXNIT®:OX-V2



2pin-contactor & double O-ring type

Avoid putting both DO probe and pH electrode together in the same sample water.

Measuring range	
DO mode	DO:0.00~30.00mg/ℓ Oxygen in the air:0.0~30.0% Water temperature:0.0~50.0℃
pH mode	pH:0.00~14.00 mV:-1900~+1900mV ORP:-1900~+1900mV Water temperature:0.0~50.0℃

Collecting water measurement	Throw-in measurement pH electrode
CE-106 standard	CE-120-3 by your instruction

10 F-10Z

Fluoride Ion Meter



■ Automatic measuring range switch function

Measuring method	Solid membrane fluoride Ion Electrode Method
Measuring range	0~2000mg/ℓ
resolution	0.1mg/ℓ (0.1~99.9)
	1mg/ℓ (100~2000)

Usage

Semi-conductor mfg. plant, glass plant, fluoride resin mfg. process, plant drainage, city water system, etc.

11 CL-10Z

Chloride Ion Meter



■ Automatic measuring range switch function

Measuring method	Solid membrane Chloride Ion Electrode Method
Measuring range	0~2000mg/ℓ
resolution	0.1mg/ℓ (0.1~99.9)
	1mg/ℓ (100~2000)
Selectivity	Unable to co-exist with S,CN

Usage

Septic tank drainage, plant drainage, food and chemical plant, etc.

12 CLCU-55

Chloride Ion Meter

Chloride Meter for Copper plating Solution without influenced Copper or $CuSO_4$



Product Name	Chloride Ion Meter	
Model	CLCU-55(for High Density)	CLCU-55L(for Low Density)
Measuring Method	Chloride Ion Measurement in Copper Plating Liquid	
Measuring Range	0.0~199.9mg/ℓ	0.00~19.99mg/ℓ
Resolution	0.1mg/ℓ	0.01mg/ℓ
Measuring time	Approx. 3 min.	
Power Supply	Alkaline battery LR03×4(DC 6V)	
Outer Dimensions	88(W)×174(D)×65(H)mm	
Standard Components	Instrument, Measuring cell(4pcs), Reagent:CLCU-RA-H 500mℓ(50 tests), Carrying Case, Micro-Pipette 100μℓ Chloride Ion standard Solution : 50mℓ	
Optional Accessories	Macro-Pipette 10mℓ, Filter Paper	

13 10Z Set

Water quality testing set

Septic tank doctor's water quality inspection kit
9 items inspection by single unit **[10Z-2]**



Easy to carry.




Convenient water holding kit
(with SUS basket)

No.	Product name	Single model	Set model	
			10Z-1	10Z-2
1	DO Meter	DO-10Z	●	●
2	pH/ORP Meter	KP-10Z	●	●
3	Chloride Ion Meter	CL-10Z	●	●
4	Chlorine Tester	DP-1Z		●
5	Transparency Meter	30cm		●
6	SV Cylinder	1ℓ		●
7	NO ₂ Reactor	GR reagent	●	●
8	Basket	Stainless steel		●
9	Case for 3 units		●	●

※Combination can be chosen by your needs.

14 MIZUTEPPPO® No.1

Piston-type water collector

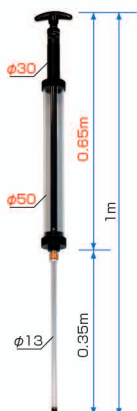


500mℓ water
collection is OK
by one time.

Water collection
at deep, narrow
or shallow place
is OK.

15 MIZUTEPPPO® No.2

Piston-type water collector

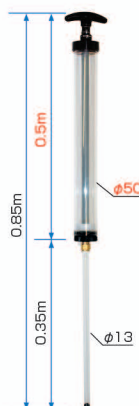

16 AT type Transparency Meter




Strong and transparent plastic-made

30cm/50cm/100cm

model	length
AT-1	30cm
AT-2	50cm
AT-3	1m


17 JT type Transparency Meter



30cm/50cm/100cm

model	Measuring range	length
JT-3	Max. 1m	30cm×2/ 40cm×1
JT-2		50cm×2


18 SV Tester SV-1000 Sludge deposit rate tester

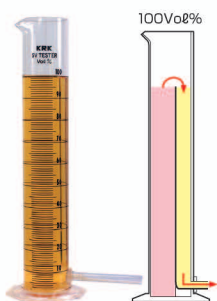

0~100%
100% level
automatic sludge
adjusting deposit
rate tester

19 Dropper type water collector

0.5m~2m
200mℓ water
collection is OK
by one time




0.5m/1m/1.5m/2m

20 ODEI-pro® No.2/No.3 Sludge Level Detector

3m/1set


Measurement of sludge surface,
water fault in various deposit tank.

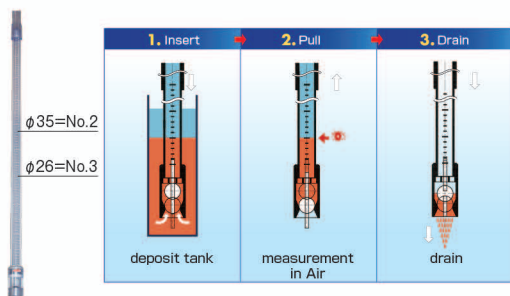

With back wash preventive function
With automatic sludge drain function

21 Scummer Z

Scum Thickness Tester

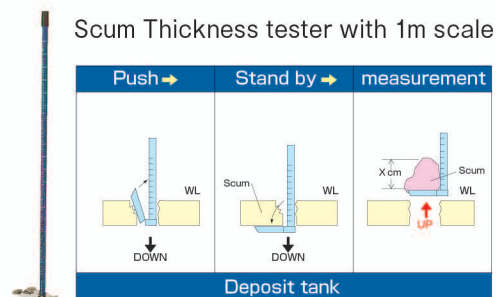

model	Type 1 : 1m Type 2 : 2m
scale	0~1m min. scale 1cm
materials	SUS-304 pipe with corrosion resistance, etc.

22 TCR-5Z

Turbidity / Colority Sensor



Measurement of turbidity and colority at the same time

Measuring range	Turbidity/colority mode 1 : 0.0~50.0 Degree
	Turbidity/colority mode 2 : 0.00~9.99 Degree
	Light absorbance mode : 0.000~1.999 Abs
Min. display	0.1⇄0.01(display switch below 10 Degree)
Measuring method	Turbidity : polystyrene turbidity,transmission light
	Colority : platinum cobalt colority standard

23 TCR-30

Turbidity / Colority Sensor



Measurement of both turbidity and colority by this single unit
Double-beam type turbidity /colority sensor

Measuring range	Turbidity/colority mode 1 : 0.0~50.0 Degree
	Turbidity/colority mode 2 : 0.00~9.99 Degree
Min. display	0.1⇄0.01(display switch below 10 Degree)
Measuring method	Turbidity : polystyrene turbidity,transmission light
	Colority : platinum cobalt colority standard

24 TR-30 Turbidity Sensor



Measuring range	0~50.0 Degree
Measuring method	polystyrene turbidity standard, transmission light method

25 CR-30 Colority Sensor



Measuring range	0~50.0 Degree
Measuring method	Platinum cobalt colority standard

Necessity of water quality control of city water, water tank, swimming pool, etc.

26 TR-5Z 90° scattered light Turbidity Sensor

Probe type Near infrared 90° scattered light Turbidity Sensor



Measuring range	0~200 Degree
Resolution	0.01 Degree(0~20)
	0.1 Degree(20~200)
Measuring unit	Formazine turbidity (NTU) standard

Measurement of 0.00~200 Degree(NTU)

27 SSTR-5Z SS / Turbidity Sensor



Near infrared
90° scattered light probe type sensor
Measurement by switching SS to Turbidity
(after confirming fixed factor)

Measuring range	Turbidity : 0.0~500 NTU
	SS : 0 ~ 500mg/ℓ (converted value)
Converting function	$y = a+bx(x=\text{turbidity}, y=\text{SS})$

28 TR-55 Scattered transmitted light Turbidity Sensor




Scattered and transmitted light measurement
Measurement from low density to high density

Measuring range	0~1100 Degree
Resolution	0.01 Degree(0~10.99)
	0.1 Degree(11.0~109.9)
	1 Degree(110~1100)
Measuring unit	Degree or FTU

29 DP-3F

DPD Method Residual Chlorine Meter

0~5mg/ℓ Measurement

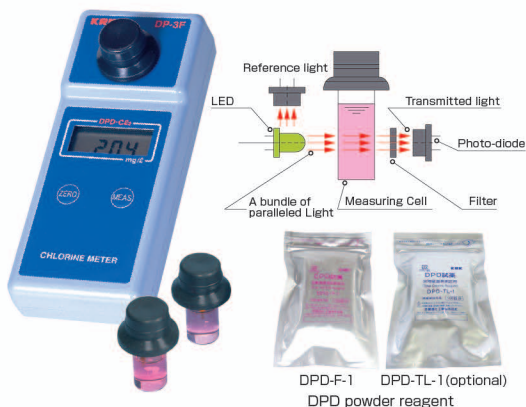

Measuring range	0~5mg/ℓ
resolution	0.01mg/ℓ (0~3)
	0.1mg/ℓ (3~5)
Measuring reagent	Free residual chloride measuring reagent : DPD-F-1 (standard)
	Total residual chloride measuring reagent : DPD-TL-1 (optional)


30 RC-3F

High density Chlorine Meter

0~300mg/ℓ Measurement



Principle Drawing

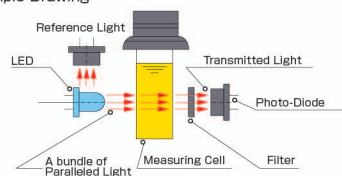

Measuring range	0~300mg/ℓ
Coloring reagent	HOC-K-1
Measuring theory	Light absorbance method by coloring reagent

31 RC-V2

Multi-range Residual Chlorine Meter

0~3mg/ℓ / 0~20mg/ℓ / 0~300mg/ℓ / 0~3000mg/ℓ / 0~200g/ℓ

Measurement from low density chlorine to high density sodium hypochlorite.



Measuring object	Chlorine disinfectant water, electrolytic hypogenerated water, city water, bath tub water, swimming water	
Measuring range	D P D mode	0.00 ~ 3.00mg/ℓ
	RC-L mode	0.0 ~ 20.0mg/ℓ
	RC-H mode	0 ~ 300mg/ℓ
	RC-T mode	0 ~ 3000mg/ℓ
	RC-U mode	0.0 ~ 200.0g/ℓ

32 O₃-3F

Dissolved Ozone Meter

Measurement of dissolved ozone in the water within 0~3 mg/ℓ



OZ-K-1
Reagent for
ozone test

Measuring Operation



Measuring range	0.00~3.00mg/ℓ
Measuring object	Ozone treated city water, etc.
Measuring purpose	Sterilization, ozone density control and measurement of sterilizing process.
Measuring reagent	OZ-K-1

33 TP-10Z Transparency Sensor

Probe type
Digital display,
Electronic Transparency Sensor



Transparency mode
(example)

32.0
cm

Change mode

Absorbance mode
(example)

0.106
Abs

34 TP-30 Transparency Sensor

Combined type



Filter for
calibration
attached as
standard


Wave length	Near Infrared Ray(880nm)
Display	LCD 4 digits
Range	Transparency :2.0~200cm Absorbance :0.000~2.000Abs/60mm
Minimum resolution	0.1cm (2.0~99.9cm) 1cm (100~200cm) 0.001Abs
Accuracy	Within ±3% (FS) (at fixed condition)
Calibration	① Simple calibration filter ② Equivalent standard solution for calibration

Wave length	Near Infrared Ray(880nm)
Range	2.0~200cm
Display	LCD 3 digits
Minimum resolution	0.1cm (2.0~99.9cm) 1cm (100~200cm)
Accuracy	Within ±3% (FS) (at fixed condition)
Calibration	① Simple calibration filter ② Equivalent standard solution for calibration


35 CHL-30

Chlorophyll Sensor

<Fluorescence strength sensor>

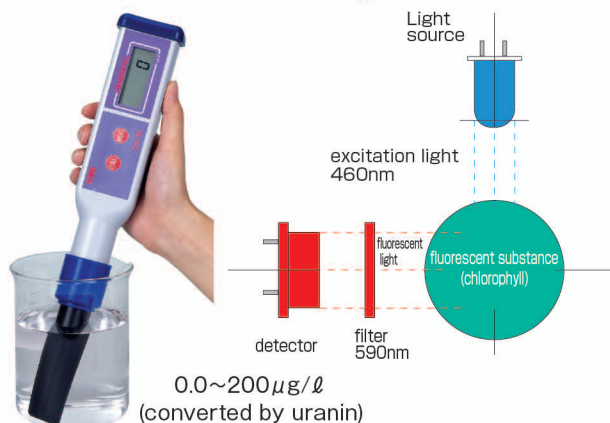

Correlation between uranin converted fluorescence quantity and chlorophyll

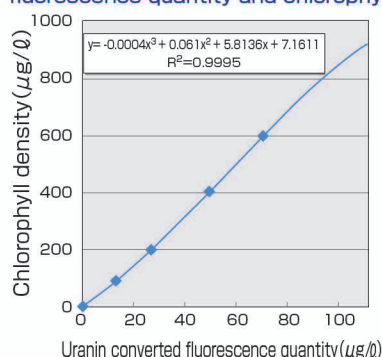


36 CHL-5Z

Chlorophyll Sensor

Measurement of fluorescence strength of phytoplankton's chlorophyll.



Correlation between uranin converted fluorescence quantity and chlorophyll

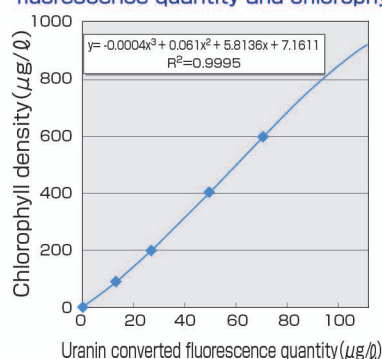

37 EC-5Z

Electric Conductivity Meter

Measurement of EC, salt, water temp. by a single unit



- ◇ Convenient to switch from **SI unit** (mS/m) to **old unit** (mS/cm)
- ◇ Chemical-proofed carbon EC sensor

Measuring method	AC 2 electrode Method	
Measuring range	EC-5Z-H	EC-5Z-L
SI unit	0~20S/m	0~2S/m
Old unit	0~200mS/cm	0~20mS/cm
Cell constant	$\theta=400\text{m}^{-1}$	$\theta=100\text{m}^{-1}$

38 LQ-5Z Electrode type liquid density Meter



With this sensor, you can measure liquid density without using any reagent.

■LQ-5Z series

TMAH meter	LQ-5Z-TMAH	0.00~5.00%
Sulfuric acid meter	LQ-5Z-H ₂ SO ₄	0.00~2.00%
Nitric acid meter	LQ-5Z-HNO ₃	0.00~2.00%
Sodium hydroxide meter	LQ-5Z-NaOH	0.00~3.00%
Potassium hydroxide meter	LQ-5Z-KOH	0.00~3.00%
Ammonium sodium meter	LQ-5Z-NH ₃	0.00~2.00%


39 Cu-V2 Copper Ion Meter

Water quality inspection of Copper Ion for plating & Etching Process




Model	Cu-V2
Measuring object	Copper Ion
Measuring Method	Reduction and Bicinchoninic Acid Method
Measuring range	Copper Ion :0.00~10.00mg/ℓ (Cu ^T) Absorbance:0.000~2.000Abs
Repeatability	Within ±2%(FS)
Memory function	Max19 Data
Standard Component	Instrument,measuring Cell(4pcs) Reagent(Cu-V2-RA):50tests Carring Case,Spoit

■Copper Ion & Abs can be measured with one single instrument



■With memory Function



■Bicinchoninic Acid Method Reagent



40 Ni-V2**Nickel Ion Meter**

Water quality inspection of Nickel Ion for plating Process



■ Nioxime Method Reagent



Model	Ni-V2
Measuring object	Nickel Ion
Measuring method	Nioxime Method
Measuring range	Nickel Ion : 0.00~10.00mg/ℓ (Ni^{2+}) Absorbance: 0.000~2.000Abs/cm
Repeatability	Within $\pm 2\%$ (FS)
Memory function	Max19 Data
Standard Component	Instrument, measuring Cell (4pcs) Reagent (Ni-V2-RA): 50 tests Carrying Case, Spoit

■ Nickel Ion & Abs can be measured with one single instrument



MODE



Nickel



absorbance

41 H₂O₂-V series Hydrogen peroxide density Meter H_2O_2 measurement of plating liquid, etching liquid and disinfectant liquid

	High density	Medium density	Low density
Model	H ₂ O ₂ -V1	H ₂ O ₂ -V2	H ₂ O ₂ -V3
Measuring object	H ₂ O ₂ in copper plating liquid		H ₂ O ₂ in disinfectant liquid
Measuring range	0.0~120.0g/ℓ	0~1200mg/ℓ	0.00~25.00mg/ℓ
Measuring time	Approx. 1 minute		
reagent	1 kind (with 50 pieces)		

42 H₂SO₄-55**Sulfuric Acid Meter**Measurement of H_2SO_4 Density for Plating & Etching Process LiquidPossible to measure Sulfuric Acid
Density by 0-199g/ℓ

Model	H ₂ SO ₄ -55
Measuring Method	Light Absorbance Method
Measuring Range	0.0~199.9g/ℓ (H_2SO_4)
Display	LCD 3·1/2 digits
Standard Components	Instrument (H ₂ SO ₄ -55), Measuring cell (4pcs) Reagent : H ₂ SO ₄ -RA 500mℓ (50 tests), Carrying Case. Micro-Pipette 100μℓ

43 CU-5Z

Copper Meter



- ◇ Copper density measurement of copper sulfate plating solution, etching solution
- ◇ Copper sensor not influenced by sulfuric acid nor hydrogen peroxide
- ◇ Sensor is PFA treated and chemical-proofed

■ Measurement of 3 selective mode

Copper density	Cu: 0.0~76.3g/ℓ
Copper sulfate	CuSO ₄ : 0~300g/ℓ
Mole density	0.000~1.200mol/ℓ

44 Ni-5Z / Ni-5ZL

Nickel Meter

Measurement of Nickel density at plating process



Model	High density Ni-5Z	Low density Ni-5ZL
Measuring range	0.0~199.9g/ℓ	0.00~19.99g/ℓ

■ Usage

Nickel density measurement of nickel sulfate solution, nickel sulfamate solution

45 CuNi-5Z

Copper/Nickel Meter

Copper and Nickel density of copper sulfate or Nickel plating solution by this single unit



Measuring range	Copper density	Cu: 0.0~80.0g/ℓ
	Copper sulfate	CuSO ₄ : 0.0~300g/ℓ
	Nickel density	Ni: 0.0~199.9g/ℓ

Colorimetric Tester (Aqua Tester, DPD reagent)

46 1Z/2Zseries (9-grade measurement)



■ Colorimetric disk series



Multi item water quality measurement is available with this single unit by changing the colorimetric disks and reagents.

1Z/2Z series (9-grade measurement)

Measuring item	model	Measuring range
Residual chlorine(DPD)	DP-1Z	0.05~2.0mg/ℓ
pH/ Residual chlorine	DP-2Z	0.05~2.0mg/ℓ
		6.0~7.6pH
High Density chlorine	CL2-1Z-H	10~150mg/ℓ (20~300mg/ℓ)
pH(BTB)	BTB-1Z	6.0~7.6pH
pH(BTS)	BTS-1Z	5.8~8.6pH
pH(BTM)	BTM-1Z	5.0~9.0pH
Dissolved ozone	O3-1Z	0.1~1.5mg/ℓ
Ammonium nitrogen	NH4-N-1Z	0.2~10.0mg/ℓ
Nitric nitrogen	NO2-N-1Z	0.006~0.3mg/ℓ
Nitrate nitrogen	NO3-N-1Z	0.05~4.5mg/ℓ
Phosphate	PO4-1Z-T	0.2~5.0mg/ℓ
H. phosphate	PO4-1Z-H	10~240mg/ℓ
COD	COD-2Z	5~100mg/ℓ
		1~25mg/ℓ
Total iron	Fe-1Z	0.1~5.0mg/ℓ
Manganese	Mn-1Z	0.5~20.0mg/ℓ
Total copper	Cu-1Z-N	0.1~10mg/ℓ
Chromium hexavalent	Cr-1Z	0.05~10mg/ℓ
Free cyanide	CN-1Z	0.01~5mg/ℓ
Nickel	Ni-1Z	0.3~10mg/ℓ
Zinc	Zn-1Z	0~5mg/ℓ
Formaldehyde	HCHO-1Z	0~2mg/ℓ

47 7Zseries (10-grade measurement)



7Z series (10-grade measurement)

Measuring item	model	Measuring range
Residual chlorine(DPD)	DP-7Z	0.05~2.0mg/ℓ
Available chlorine	RC-7Z	10~200mg/ℓ
pH(BTB)	BTB-7Z	5.8~7.6pH
pH(BTS)	BTS-7Z	5.8~8.6pH
pH(BTM)	BTM-7Z	4.5~9.0pH
Total hardness	TH-7Z	5~300mg/ℓ

48 DPD measuring reagent for Residual Chlorine

Line-ups of separately packed powder reagent and liquid reagent.



DPD-WA-50 DPD-WA-18 DPD-F-1 DPD-TL-1
DPD liquid reagent DPD powder reagent

NEW

**DPD Reagent,
Liquid Type**

For Free Chlorine



DPD-GL

- Just one drop for Free Residual Chlorine Measurement
- Long-Term storable DPD Liquid Reagent
- A Mere one drop, add it, so rapid Measurement
- Assorted Waste-Free DPD Liquid Reagent

Product Name	DPD Reagent, Liquid Type
Object	Free Chlorine
Model	DPD-GL-10(10mℓ)
Volume	10mℓ (approx 200 Times)
Using Volume	1 Drops/1 time(approx:0.05mℓ)
Optional	DPD-GL-25(approx:500 times)

49 700/800series Field installing type, industrial water quality Meters



Field Installing Type 700/800 series

Product name	Model	Measuring range
pH Meter	PC-700	0.00~14.00pH
ORP Meter	OC-700	0~±1900mV
DO Meter	DC-700	0.00~20.00mg/ℓ
Turbidity Meter	TR-700Z	0.0~500 Degree
MLSS Meter	MC-700	0~20000mg/ℓ
Electromagnet Density Meter	EMC-700	0.0~20.0%(NaCl)
Electric Conductivity Meter	EC-700	0~20S/m
SS/Turbidity Meter	TSS-700W	0~1000(FTU or mg/ℓ)
Turbidity/Colority Meter	TCR-700W	Turbidity 0~50 Degree Colority 0~50 Degree
Copper Meter	CU-800	0.0~80.0g/ℓ Cu
Nickel Meter	Ni-800	0.0~200.0g/ℓ Ni


50 502/301series Panel Installing Type



Panel Installing Type 502/301 series

Product name	Model	Measuring range
pH Meter	PC-502	0.00~14.00pH
ORP Meter	OC-502	0~±1900mV
DO Meter	DC-502G	0.00~20.00mg/ℓ
Turbidity Meter	TR-502Z	0.0~500Degree
MLSS Meter	MC-502	0~20000mg/ℓ
Electromagnet Density Meter	EMC-502	0.0~20.0%(NaCl)
Electric Conductivity Meter	EC-502	0~20S/m
Colority Meter	CR-502	0~50 Degree
Turbidity/Colority Meter	TCR-502	Turbidity 0~50 Degree Colority 0~50 Degree
Copper Meter	CU-502	0.0~80.0g/ℓ Cu
Nickel Meter	Ni-502	0.0~200.0g/ℓ Ni
Chlorine Meter	RC-301Z	0~2mg/ℓ Cl ₂


Detectors for Process Measurement

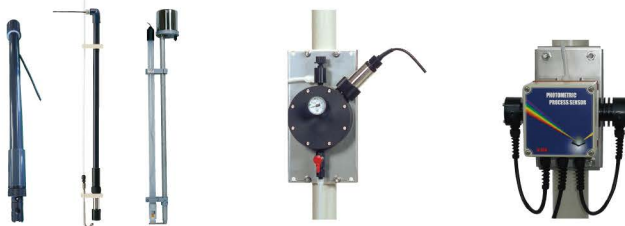

51 UV-700W

UV/COD Monitor

Prove type UV/LED detector With cleaning wiper

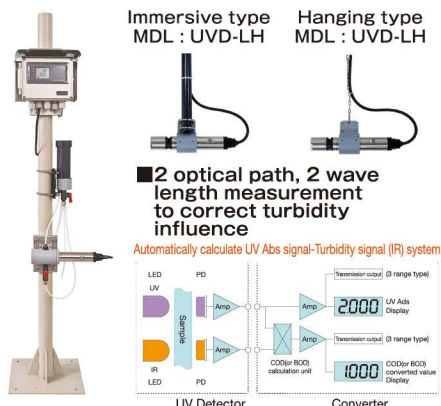


Specifications of converter

Product Name	UV organic pollution monitor(UV/COD Monitor)
Model	Standard Type :UV-700W-10 (CELL length:10mm) High Density Type:UV-700W-5 (CELL length:5mm)
Display	LCD 4-digits 2 Steps, Upper:COD converted value Lower:UV Abs(255nm)
Measuring Range	[UV-700W-10] UV:0~2.000Abs/cm COD(cr):0~500mg/ℓ (converted Value):MAX [UV-700W-5] UV:0~4.000Abs/cm COD(cr):0~1000mg/ℓ (converted Value):MAX △Attention:Depending upon the water quality,conversion Measurement can not be made below500 or 1000mg/ℓ (cr)
Transmission output	4~20mA DC 2 system,3 range switch

52 TSS-700W

SS/Turbidity Sensor

With cleaning wiper

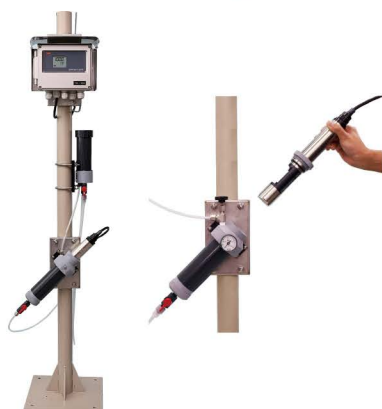

Meter

Model	TSS-700W-20(STD)/TSS-700W-60(Low density)
Measuring unit	Formazine Turbidity(FTU)or SS mg/ℓ (instruct us Measuring unit at the time of order)
Measuring range	TSS-700W-20:0.1~1000 degree TSS-700W-60:0.01~50 degree
Transmission output	4~20mA DC(isolation type)
Accuracy	Within ±2%(FS)


SS/turbidity detector TSSD-20W

Measuring theory	Near infrared rays transmission light
Detector model	TSSD-20W(STD)/TSSD-60W(Low density)
Cleaning wiper	Wiper built-in detector
Optical path	20mm(STD) or 60mm(for Low density)

53 TCR-700W

Turbidity/Colority Monitor

Simultaneous Measurement and display of both Turbidity and Colority

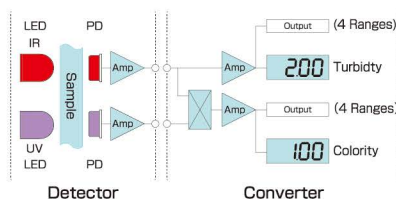


Meter

Measuring range	Turbidity: 0~50degree(FTU or mg/ℓ) Colority: 0~50degree(Pt cobalt degree)
Resolution	0.01degree(at under 10),0.1degree(at 11~50degree)
Transmission output	DC4~20mA 4range(Manual change) 0~5/0~10/0~20/0~50
Accuracy	±0.1degree/at Full Scale 10degree

54 TR-502L Turbidity Monitor of Laser scattered Light Method


Laser scattered light method, sensitive turbidity detector
Sensitive of 0.001 measurement of 0.000~2.000

Measuring Diagram

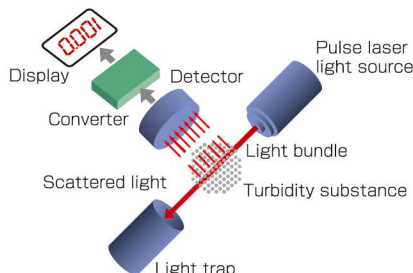

If 660nm red pulse laser bundle is projected into the sample water, strong scattered light occurs. This scattered light is detected by the light receiving element angled at 90°, transferred to the converter as density signal, calculated, amplified and digitally displayed. Laser turbidity monitor sensitively measures molecule turbidity little influenced by colority.

Linearity features

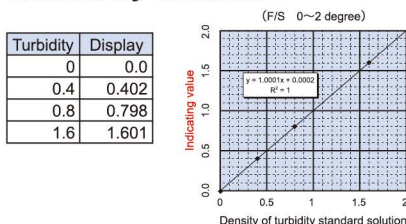

TRDH-5L

- Laser scattered light method, sensitive turbidity detector
Sensitive of 0.001 measurement of 0.000~2.000
- 3-range manual selection of transmission output
0~0.5/0~1.0/0~2.0
- Either PSL or formazine turbidity is possible to measure
- Simple and reliable zero calibration
- Simple and reliable span calibration
- Detector and converter of simple fixing and instrumentation
- With function of checking list of detector's trouble and calibration

55 DC-502G DO Monitor



OXNIT OX-VW2

OXNIT OX-VW2

NEW DO SENSER
OXNIT® **OX-VW2**

※OXNIT is the KASAHARA's registered trademark.

- Sensor cartridge is easily replaced and maintained



Meter

Measuring range	0.00~19.99mg/ℓ
Resolution	0.01
Power supply	AC85~240V 50/60Hz
Transmission output	DC4~20mA (insulation type) Range1: 0.00~5.00mg/ℓ Range2: 0.00~10.00 mg/ℓ Range3: 0.00~19.99 mg/ℓ (Initial setting)

DO Detector

Product Name	Galvanic DO Detector
Measuring Method	Cartridge type DO Sensor
Model	Immersion Type DO Probe : OXP-2VNY-H DO Sensor : OXNIT[OX-VW2] Throw in Type DO Probe with sinker : OXP-2VNY-SK DO Sensor : OXNIT[OX-VW2]



KRK

KASAHARA CHEMICAL INSTRUMENTS CORP.

2-133-8 SAKURADA KUKI-CITY SAITAMA JAPAN
〒340-0203

TEL:0480-38-9151 FAX:0480-38-9157

URL:<https://www.krkjpn.co.jp>